

Medical Grade AC/DC Power Supply With PFC

85-264 Vrms 12/24/36/48 V 300 W 400 W Up to 91 %
Input Voltage Semi-Regulated Output Output Continuous Output Transient Full Load Efficiency



Product Features

- High efficiency (91% for 48 Vout Model at 300 W)
- Universal input voltage range
- Semi-regulated output for bus stability
- Parallel operation supported
- Integral fan cooling with speed control
- Active PFC; EN61000-3-2 compliant
- Low leakage; EN60601-1 compliant
- Low noise; EN55011 / EN55022 Class B compliant
- Medical EMI Compatibility: IEC 60601-1-2 ed 4.0 compliant

- Over-current, over-voltage, & over-temp protection
- DC Power Good / AC Power Good signals
- Remote enable input
- Fan status output / Fan enable input
- Small size: 3" x 5" x 1.45"(open frame)
- RoHS 6/6 compliant
- 5 V (10 W) and 12 V (50 W) standby outputs

ACuQor 300 W Triple Vout Series Electrical Characteristics All specifications typical with T_A = 25 °C, unless otherwise specified. Specifications subject to change without notice.

0 °C to +70 °C to +85 °C +70
-40 °C to +85 °C 5-95% RI 10,000 ft may 30,000 ft may 0.03 g2/H 20 g pea 6 Level Class Clause 5 Level 4, +/-15k' AC Input Connection DC Output Connection Level 4, +/-8k' teria A; HCP, VCP, Cas Level 3, 10V/r 50601-1-2 Ed.4 Table 28 V/r
5-95% RI 10,000 ft max 30,000 ft max 0.03 g2/H 20 g pea 6 Level Class a Clause 5 Level 4, +/-15k AC Input Connection DC Output Connection Level 4, +/-8k teria A; HCP, VCP, Cas Level 3, 10V/r 50601-1-2 Ed.4 Table 28 V/r
10,000 ft may 30,000 ft may 0.03 g2/H 20 g pea Class . Clause 5 Level 4, +/-15k AC Input Connection CO Output Connection Level 4, +/-8k teria A; HCP, VCP, Cas Level 3, 10V/r 50601-1-2 Ed.4 Table 28 V/r
30,000 ft may 0.03 g2/H 20 g pea Class Clause 5 Level 4, +/-15k AC Input Connection CO Output Connection Level 4, +/-8k teria A; HCP, VCP, Cas Level 3, 10V/r 50601-1-2 Ed.4 Table 28 V/r
0.03 g2/H 20 g pea 6 Level 1 Class . Clause 5 Level 4, +/-15k , AC Input Connection DC Output Connection Level 4, +/-8k teria A; HCP, VCP, Cas Level 3, 10V/r 50601-1-2 Ed.4 Table 28 V/r
20 g pea Class . Clause 5 Level 4, +/-15k , AC Input Connection DC Output Connection Level 4, +/-8k teria A; HCP, VCP, Cas Level 3, 10V/r 50601-1-2 Ed.4 Table 28 V/r
Clause 5 Clause 5 Level 4, +/-15k' AC Input Connection CO Output Connection Level 4, +/-8k' teria A; HCP, VCP, Cas Level 3, 10V/r 50601-1-2 Ed.4 Table 28 V/r
Clause 5 Clause 5 Level 4, +/-15k' AC Input Connection CO Output Connection Level 4, +/-8k' teria A; HCP, VCP, Cas Level 3, 10V/r 50601-1-2 Ed.4 Table 28 V/r
Class A Clause 5 Level 4, +/-15k' AC Input Connection DC Output Connection Level 4, +/-8k' teria A; HCP, VCP, Cas Level 3, 10V/r 50601-1-2 Ed.4 Table 28 V/r
Clause 5 Level 4, +/-15k' AC Input Connection OC Output Connection Level 4, +/-8k' teria A; HCP, VCP, Cas Level 3, 10V/r 50601-1-2 Ed.4 Table 28 V/r
Level 4, +/-15k, AC Input Connection CO Output Connection Level 4, +/-8k, teria A; HCP, VCP, Cas Level 3, 10V/r 50601-1-2 Ed.4 Table 28 V/r
, AC Input Connection DC Output Connection Level 4, +/-8k teria A; HCP, VCP, Cas Level 3, 10V/r 50601-1-2 Ed.4 Table 28 V/r
, AC Input Connection DC Output Connection Level 4, +/-8k teria A; HCP, VCP, Cas Level 3, 10V/r 50601-1-2 Ed.4 Table 28 V/r
OC Output Connection Level 4, +/-8k teria A; HCP, VCP, Cas Level 3, 10V/r 50601-1-2 Ed.4 Table 28 V/r
Level 4, +/-8k teria A; HCP, VCP, Cas Level 3, 10V/r 50601-1-2 Ed.4 Table 28 V/r
teria A; HCP, VCP, Cas Level 3, 10V/r 50601-1-2 Ed.4 Table 28 V/r
Level 3, 10V/r 50601-1-2 Ed.4 Table 28 V/r
50601-1-2 Ed.4 Table 28 V/r
28 V/r
Perf Criteria
Level 3
(Hz rep, AC input lead
50601-1-2 Ed.4 Table
Perf Criteria
Level
Perf Criteria
Level
Perf Criteria
30 A/r
50601-1-2 Ed.4 Table
Perf Criteria
0% Ut
5 cycle 45° increment
0% Ut; 1 cycl
70% Ut; 0.5
50601-1-2 Ed.4 Table
eria A, Load Depender
0% Ut; 5
50601-1-2 Ed.4 Table
Perf Criteria
Terr criteria
500 kH
250 kH
39 dBA @ 1 m max
1 oz) \ 446 g (15.7 oz
343.6 kHour
TBD kHour
TDD KHOUI
4000 17
4000 Vrm
4000 Vrm
4000 Vrm 1500 Vrm
1500 Vrm 1500 Vrm
1500 Vrm 1500 Vrm 5000 Vpuls
1500 Vrm 1500 Vrm
66

- 1. Main output power rating always includes 5 V and 12 V standby outputs.
- 2. Leakage currents see following table.

EMC Immunity Testing Details

ESD EN61000-4-2

For ESD tests applied directly to the DC output, one of the methods called out in IEC 61000-4-2 section 7.1.3 must be used to bleed off charge between successive ESD events. For example, the cable with 2 x 470kOhm resistors used for this purpose during coupling plane tests can be duplicated and connected from DC output to protective earth (PEGND).

Discharges must not be applied directly to any circuits other than the case (for encased models), the AC input connections, and the DC output connections. For ESD protection in equipment, it is important to follow the ACuQor Installation Instructions provided with each unit in regards to clearance. Those instructions are repeated here for emphasis. CF and CFD models, in particular, may experience high DC output voltages with respect to protective earth (PEGND) due to their low capacitance/low-leakage design if ESD pulses are directly applied. Maintaining adequate clearance will prevent arcing from ACuQor DC output circuitry to other user circuits and chassis.

Voltage Dips EN61000-4-11

The following table details the DC output loading conditions and performance criteria for AC input voltage dip tests.

ACuOor 300/400/500W Performance

Test Condition	DC Load	Criteria
0% UT; 0.5 cycle at 0, 45, 90, 135, 180, 225, 270 and 315 degrees	0 to 400 W	Α
	> 400 W	В
0% UT; 1 cycle at 0 degrees	0 to 350 W	Α
	> 350 W	В
70% UT; 25/30 cycles (0.5s) at 0 degrees	0 to 450 W	Α
	> 450 W	В
0% UT; 250/300 cycles (5s) at 0 degrees	All loading	В

Note: 300W models limited to 400W transients

Leakage Currents

AC Leakage Current from Input to Earth	AC Line Connection	Normal Condition	Open Neutral Fault
ACuQor Typical at	240 V L-N, 1 phase	125 μΑ	250 μΑ
	208 V L-L, 120 V L-N, 1 of 3 phases	65 µA	130 μΑ
	240 V L-N-L, 120 V L-N, split phase	65 µA	130 μΑ

AC Leakage Current from Output to Earth		Normal Condition	Open Earth Fault	AC Backdrive Fault
ACuQor Typical at 264 Vac 60 Hz input	AQ BF	2 μΑ	36 μΑ	125 μΑ
	AQ CF	2 μΑ	6 μΑ	18 μΑ

For convenience, the following tables show limits allowed by various standards:

AC Leakage Current from Input to Earth	Standard	Normal Condition	Open Neutral Fault
Maximum Allowed per Standard	IEC60601-1	500 μA	1000 μΑ
	NFPA 99 2005	300 µA	_
	IEC60950	3500 μA	_

AC Leakage Current from Output to Earth	Contact Type	Normal Condition	Open Earth Fault	AC Backdrive Fault
Maximum Allowed per IEC60601-1	BF	100 μΑ	500 μΑ	5000 μA
	CF	10 μΑ	50 μΑ	50 μΑ

Table 1: Leakage Currents

Standard Testing Certifications

•
SAFETY AGENCY CERTIFICATIONS
UL 60601-1
CAN/CSA C22.2 No. 601.1-M90
EN 60601-1
IEC 60601-1
ANSI/AAMI ES60601-1
CE Marked
Moets NEDA 90 2005 300 uA earth leakage



CONNECTOR DETAILS

Pin 11 REMOTE_ENABLE


Pin 12 12V_STANDBY

Pin 13 VOUT(-)

Pin 14 VOUT(-)

Pin 15 VOUT(-)

Pin 16 VOUT(-)



OUTPL	JT CONNECTOR PIN	OUT (top side)		
Pin 1	FAN_GOOD	Open collector with internal 5V pullup. See Figure A. Pulsed low on fan failure, 100ms, 50% duty. Short to VOUT(-) to disable fan.		
Pin 2	AC_POWER_GOOD	Open collector with internal 5V pullup. See Figure B. Pulled low on AC power dropout.		
Pin 3	DC_POWER_GOOD	Open collector with internal 5V pullup. See Figure B. Pulled low during startup ramp and within 5 $^{\circ}\text{C}$ of temperature shutdown threshold.		
Pin 4	5V_STANDBY	5 V @ 10 W available whenever AC power is applied.		
Pin 5	VOUT(+)	Positive Output Voltage.		
Pin 6	VOUT(+)	Positive Output Voltage.		
Pin 7	VOUT(+)	Positive Output Voltage.		
Pin 8	VOUT(+)	Positive Output Voltage.		
Pin 9	Reserved	Reserved for future use.		
Pin 10	Reserved	Reserved for future use.		

Logic input. See Figure C.

Negative Output Voltage. Negative Output Voltage.

Negative Output Voltage.

Negative Output Voltage.

Pull high to enable main output.

12 V @ 50 W available whenever AC power is applied.

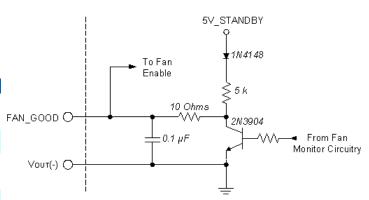


Figure A: Fan status output / Fan enable input interface circuitry.


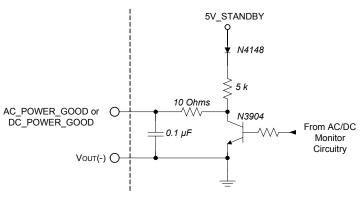


Figure B: Power good interface circuitry.



12 V	OUTPUT CONNECTOR	R PINOUT (bottom side)
Pin 1	VOUT(+)	Positive Output Voltage.
Pin 2	VOUT(+)	Positive Output Voltage.
Pin 3	VOUT(+)	Positive Output Voltage.
Pin 4	VOUT(+)	Positive Output Voltage.
Pin 5	VOUT(-)	Negative Output Voltage.
Pin 6	VOUT(-)	Negative Output Voltage.
Pin 7	VOUT(-)	Negative Output Voltage.
Pin 8	VOUT(-)	Negative Output Voltage

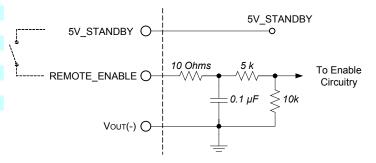



Figure C: Remote enable interface circuitry.

		3	
INDIV	IDUAL INPUT (CONNECTOR PINOUT	
Pin 1	Ground		
Pin 3	AC Neutral		
Pin 5	AC Line		

MATING CONNECTORS		
Connector	Туре	Contact
OUTPUT (16 pins)	Molex 430251600	Molex 430300008*
12V_OUTPUT (8 pins)	Molex 436450800	Molex 430300008*
INPUT	JST VHR-5N	JST SVH-41T-P1.1

* Each contact rated for a maximum of 5.5 A.

EFFICIENCY, DERATING, AND VOUT DROOP CURVES

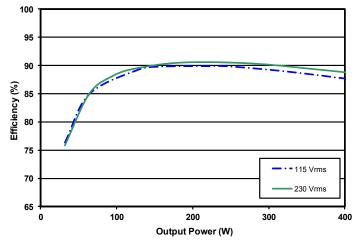

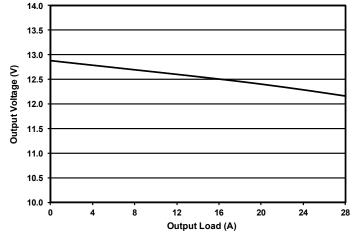
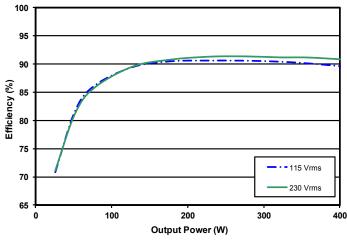


Figure 1: 12 V_{OUT} efficiency curves.

Figure 2: 12 V_{OUT} droop characteristic.





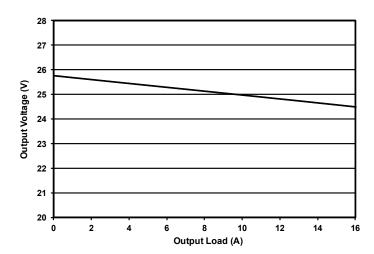


Figure 3: 24 $V_{\rm OUT}$ efficiency curves.

Figure 4: 24 $V_{\scriptscriptstyle OUT}$ droop characteristic.

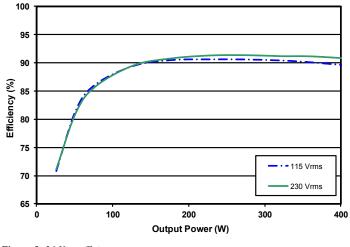

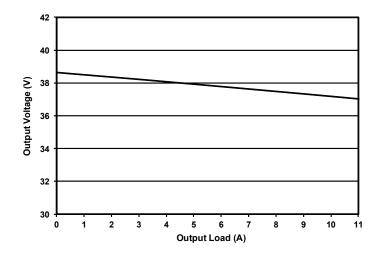

 $\textbf{\textit{Figure 5: } 36\ V_{OUT} efficiency\ curves.} \qquad \qquad \textbf{\textit{Figure 6: } 36\ V_{OUT} droop\ characteristic.}$

EFFICIENCY, DERATING, AND VOUT DROOP CURVES

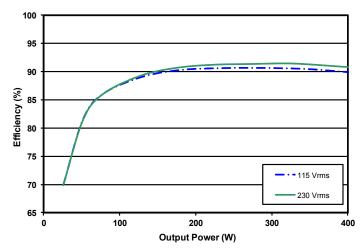


Figure 7: 48 V_{OUT} efficiency curves.

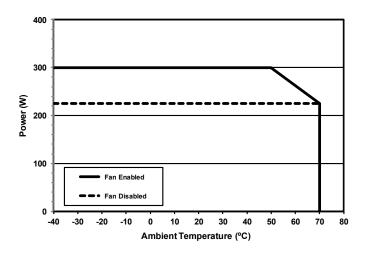


Figure 9: Continuous power derating curve in natural convection.

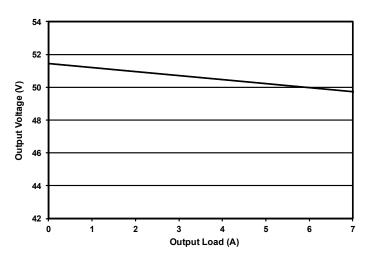


Figure 8: 48 $V_{\rm OUT}$ droop characteristic.


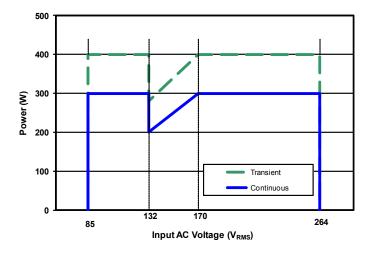



Figure 10: Rated output power vs Input AC Voltage.

MECHANICAL DRAWINGS

(1 Module Open Frame Version — E Package Type)

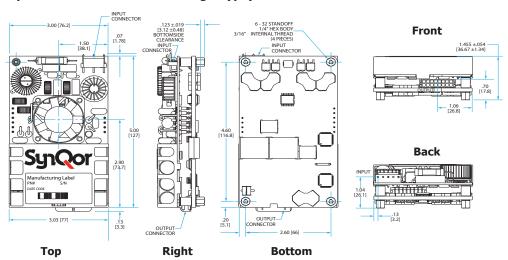

(1 Module Encased Version — E Package Type)

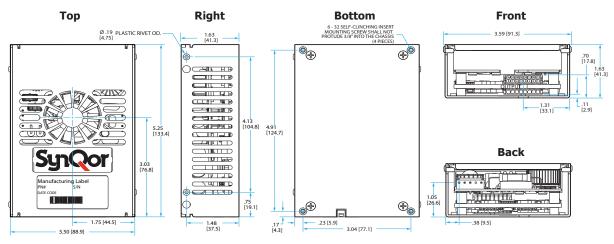

NOTES (applies to all mechanicals)

- 1) Recommended screw tightening torque of 6 in.lbs
- 2) Undimensioned components are shown for visual reference only
- 3) All dimensions in inches [mm]

Tolerances: x.xx in ± 0.02 x.xxx in ± 0.010



PARALLEL OPERATION - MULTIPLE UNITS

The following table summarizes the recommended wiring to operate multiple units in parallel. As a rule, units wired in parallel behave the same as single units. Any specification will remain unchanged that is expressed in units of voltage, time, frequency, or efficiency. Specifications expressed in terms of power, current, or capacitance, should be scaled by the number of units wired in parallel.

ACuQor units are individually calibrated at the factory, so that the output voltage vs. output current characteristic is always consistent (see Vout droop characteristic figures). As such, multiple units will share output current accurately. Full current is guaranteed from a bank of multiple units wired in parallel.

Output Connector Signal	Suggested Connection	Behavior with Multiple Units
REMOTE ENABLE	Wire in parallel	Inputs activated simultaneously
FAN GOOD	W	Wired-OR outputs – can be pulled low by any unit during an abnormal condition.
AC POWER GOOD	W.	"
DC POWER GOOD	w	п
VOUT(+), VOUT(-)	w	
12V STANDBY*	w	п
5V_STANDBY	Do not wire in parallel	Fully regulated characteristic does not support current sharing. If placed in
		parallel, only the output with the highest set-point will drive current.

^{*}Note: Triple output models only.



INSTALLATION INSTRUCTIONS

General: ACuQor AC-DC power supplies are intended for use as components in medical and industrial equipment. ACuQor units must be properly installed within end use equipment before they can be safely applied as described in this document. The suitability of the ACuQor/equipment combination must be verified through end product investigation.

Mounting: Refer to the Mechanical Drawings section. ACuQor units are provided with threaded stainless-steel stand-offs or inserts for mounting. This mounting hardware is internally connected to the input connector protective-earth terminal for functional-earth EMC control. Any orientation (vertical, horizontal, etc.) may be used. Adequate air space should be provided over the fan intake (top) and exhaust (sides) to allow for exchange of cooling air. ACuQor is designed for a pollution degree 2 environment. The suitability of the enclosed ACuQor mechanical assemblies must be verified through end product investigation.

Open-frame models: A minimum of 5 mm electrical clearance should be allowed from the connector ends, the top and sides of open-frame models. A minimum 5 mil polyester Mylar film sheet attached to the mounting surface is required to allow some deflection and to meet defibrillation proof insulation requirements.

Encased models: A minimum of 5 mm electrical clearance should be allowed from the connector ends of encased models.

Input: Refer to the Connector Details section for input connector wiring. ACuQor products require a single phase AC power source of 100-240V 50/60Hz nominal. Refer to nameplate label for input current ratings. A protective-earth connection is also required. Minimum wire size of 18 AWG (0.8mm²) is recommended. Both sides of the AC line are internally fused (see table for specific models). These fuses are not user replaceable.

Input Fuses (in Both AC Lines)
Littelfuse 6.3A 250V 21606.3XEP
Littelfuse 6.3A 250V 21606.3XEP
Littelfuse 10.0A 250V 216010XEP

Output: Refer to the Connector Details section for output connector wiring and signal I/O functionality. Refer to nameplate label for output current ratings. Main DC output (Vout+, Vout-) pins should use 20 AWG (0.5mm2) wire size. Individual main output pins should not be loaded to more than 5.5 A. For currents greater than 5.5 A, multiple main output pins/wires must be used in parallel. All signal I/O pins are referenced to Vout-.

EMC: **ACuQor** products have been tested **EMC** listed specifications in the Electrical Characteristics section. However, end use equipment must be tested verify **EMC** compliance. to

Hipot Testing: ACuQor products are rated for Hipot testing levels of 1500 Vac input to protective-earth, 1500 Vac output to protective-earth, and 4000 Vac input to output. When performing the 4000 Vac input to output test, the test voltage must be balanced evenly 2000 Vac input and output to protective-earth. Two oppositely phased test voltage sources or a single test voltage source with external balancing impedances (capacitors) may be used to prevent overstressing input or output to protective-earth insulation per IEC60601-1 2005 sub clause 8.8.1 and IEC60601-1 1990 sub clause 20.4 q.

Patient Contact: ACuQor models include versions designed for BF and CF patient contact application per IEC60601-1. These ACuQor models provide reinforced insulation at the DC output voltage level and basic insulation at the 240 Vac level from output to protective-earth. Note that equipment and wiring may add to system leakage currents so that the end product must be tested for compliance. Refer to the Electrical Characteristics section for typical ACuQor input and output leakage currents. In addition, ACuQor defibrillation rated models comply with the minimum output to protective-earth creepage/clearance requirement and defibrillator pulse test of IEC60601-1.



PART NUMBERING SYSTEM

The part numbering system for SynQor's ACuQor AC/DC power supplies follows the format shown in the table below. Not all combinations make valid part numbers, please contact SynQor for availability.

Family	Output Power	Grade	Range	Output Voltage	Package Type	Thermal Design	Options
AQ: ACuQor series of AC-DC semi-regulated output power supplies	0300: 300 W 0400: 400 W 0500: 500 W	M: (Medical)	4: 4th Generation EMC Universal (85-264 VRMS)	12: 12 V 1T: 12 V / 5 & 12 V STBY 24: 24 V 2T: 24 V / 5 & 12 V STBY 36: 36 V 3T: 36 V / 5 & 12 V STBY 48: 48 V 4T: 48 V / 5 & 12 V STBY	I F · (3"x5")	A: Open frame C: Encased	Medical Grade: BF: BF isolation rating CF: CF isolation rating CFD: CF isolation rating defibrilator proof

Example: AQ0300M412TECBF

ACCESSORIES

SynQor offers a series of assemblies that can be ordered according to the table below. Mechanical drawings for these accessories are available for download in pdf format from the SynQor website.

Part Number	Description		
AQ-CBL-INPUT1C	Input mating cable with pre-stripped wire ends (36" long).		
AQ-CBL-OUT1C	Output mating cables with pre-stripped wire ends (18" long).		
AQ-CBL-OUT1CD	Same as AQ-CBL -OUT1C with an additional 8-pins connector.		
AQ-CBL-OUT2C	Output mating cable with connectors on both ends (18" long).		
AQ-CBL-OUT2CD	Same as the AQ-CBL-OUT2C with an additional 8-pins connector.		
AQ-INSUL1M	Single module bottom-side Mylar insulator for open frame mounting		
AQ-EVAL-PRL3	Evaluation board for up to three paralleled modules.		

APPLICATION NOTES

A variety of application notes and technical white papers can be downloaded in pdf format from the SynQor website.

Online Application Notes

Online Library of Technical White Papers

SynQor website.

Contact SynQor for further information and to order:

 Phone:
 978-849-0600

 Toll Free:
 888-567-9596

 Fax:
 978-849-0602

E-mail: power@synqor.com **Web**: www.synqor.com **Address**: 155 Swanson Road

Boxborough, MA 01719

USA

PATENTS

9,143,042

SynQor holds numerous U.S. patents, one or more of which apply to most of its power conversion products. Any that apply to the product(s) listed in this document are identified by markings on the product(s) or on internal components of the product(s) in accordance with U.S. patent laws. SynQor's patents include the following:

6,545,890 6,594,159 6,894,468 6,896,526 6,927,987 7,050,309 7,085,146 7,119,524 7,765,687 7,787,261 8,149,597 8,644,027

WARRANTY

SynQor offers a two (2) year limited warranty. Complete warranty information is listed on our website or is available upon request from SynQor.